


HCL-B1 Hydrogen Chloride Sensor

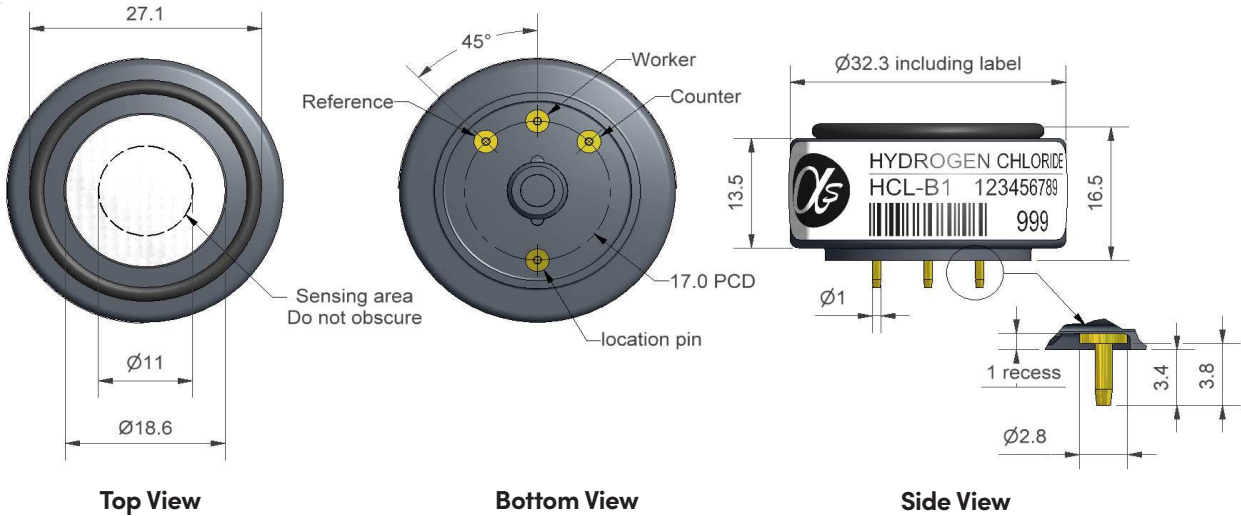

Dimensions are in millimetres (± 0.1 mm).

Performance	Sensitivity	nA/ppm in 25ppm HCl		120 to 250
	Response time	t90 (s) from zero to 25ppm HCl		< 200
	Zero current	ppm equivalent in zero air		-0.6 to 5
	Resolution	RMS noise (ppm equivalent)		< 0.1
	Range	ppm HCl limit of performance warranty		100
	Linearity	ppm error at full scale, linear at zero, 40ppm HCl		0 to 6
	Overgas limit	maximum ppm for stable response to gas pulse		200
Lifetime	Zero drift	ppm equivalent change/year in lab air		nd
	Sensitivity drift	% change/year in lab air, monthly test		nd
	Operating life	months until 80% original signal (12-month warranted)		nd
Environmental	Sensitivity @ -20°C	% (output @ -20°C/output @ 20°C) @ 25ppm HCl		60 to 90
	Sensitivity @ 50°C	% (output @ 50°C/output @ 20°C) @ 25ppm HCl		100 to 108
	Zero @ -20°C	ppm equivalent change from 20°C		< +0 to -1.0
	Zero @ 50°C	ppm equivalent change from 20°C		< +0.5 to +2.5
Cross-sensitivity	H ₂ S sensitivity	% measured gas @ 20ppm	H ₂ S	< 280
	NO ₂ sensitivity	% measured gas @ 50ppm	NO ₂	< -150
	Cl ₂ sensitivity	% measured gas @ 10ppm	Cl ₂	< -100
	NO sensitivity	% measured gas @ 50ppm	NO	< 2
	SO ₂ sensitivity	% measured gas @ 20ppm	SO ₂ (transit peak)	< 1
	CO sensitivity	% measured gas @ 400ppm	CO	< 0.1
	H ₂ sensitivity	% measured gas @ 400ppm	H ₂	< 0.1
	C ₂ H ₄ sensitivity	% measured gas @ 400ppm	C ₂ H ₄	< 0.1
	NH ₃ sensitivity	% measured gas @ 20ppm	NH ₃	< 0.1
	CO ₂ sensitivity	% measured gas @ 5%	CO ₂	< 0.1
Key Specifications	Temperature range	°C	-30 to 50	
	Pressure range	kPa	80 to 120	
	Humidity range	% rh continuous	15 to 90	
	Storage period	months @ 3 to 20°C (stored in original container)	6	
	Load resistor	Ω (recommended)	10 to 33	
	Bias voltage	mV	not required	
	Weight	g	< 13	

Figure 1 Sensitivity Temperature Dependence

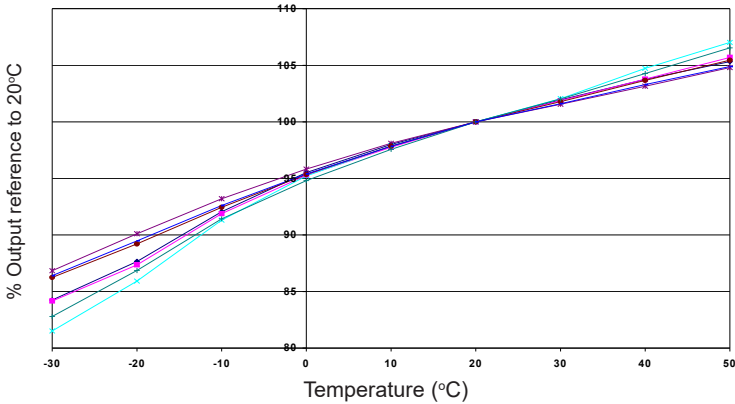


Figure 1 shows the variation of sensitivity at 25ppm HCl caused by changes in temperature.

Figure 2 Zero Temperature Dependence


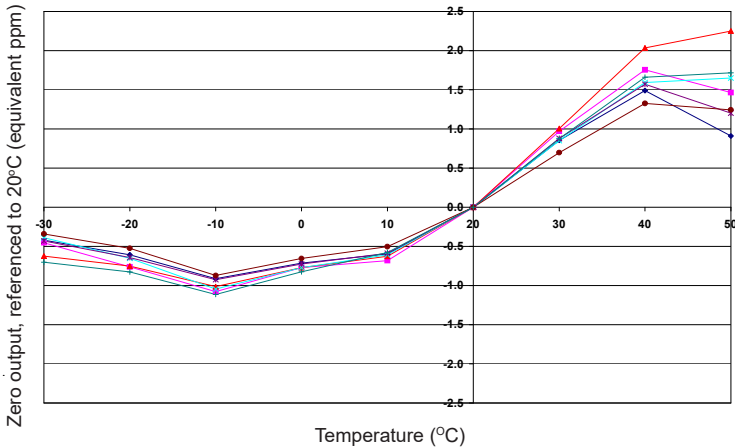


Figure 2 shows the variation in zero output caused by changes in temperature, expressed as ppm gas equivalent, referenced to zero at 20°C.
This data is taken from a typical batch of sensors.

Figure 3 Response to 200ppm HCl

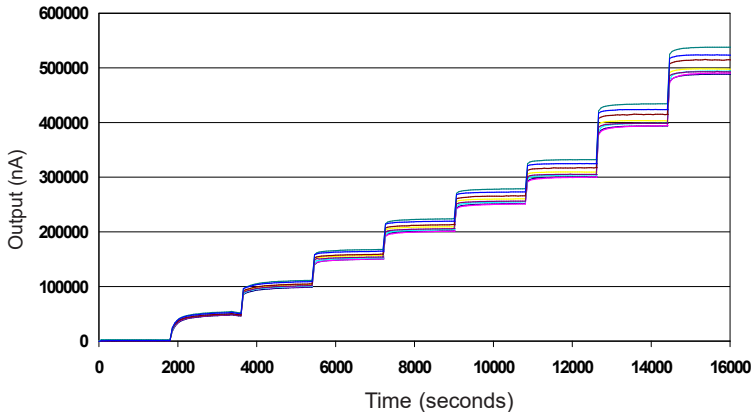

Sensor shows good response to 200ppm HCl.

At the end of the product's life, do not dispose of any electronic sensor, component or instrument in the domestic waste, but contact the instrument manufacturer, Alphasense or its distributor for disposal instructions. NOTE: all sensors are tested at ambient environmental conditions unless otherwise stated. As applications of use are outside our control, the information provided is given without legal responsibility. Customers should test under their own conditions, to ensure that the sensors are suitable for their own requirements.

In the interest of continued product improvement, we reserve the right to change design features and specifications without prior notification. The data contained in this document is for guidance only. Alphasense Ltd accepts no liability for any consequential losses, injury or damage resulting from the use of this document or the information contained within.(©ALPHASENSE LTD) Doc. Ref. HCL-B1/SEP22